

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWF-0359
Location:	LAWRENCE TWP POLICE	
Calibration File No.:	01283	Calib. Date: 09/10/2018
Certification File No.:	01284	Calib. No.: 00030
Linearity File No.:	01285	Cert. Date: 09/10/2018
Solution File No.:	01296	Cert. No.: 00026
Sequential File No.:	01296	Lin. Date: 09/10/2018
		Lin. No.: 00026
		Soln. Date: 11/04/2018
		Soln. No.: 00223
		File Date: 11/04/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWJ S3-0355
Solution Control Lot:	18050	Expires: 01/31/2020
		Bottle No.: 0619

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:14S		
Control 1 EC	0.100%	16:15S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	16:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:16S		
Control 2 EC	0.100%	16:17S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	16:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:17S		
Control 3 EC	0.100%	16:18S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	16:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:19S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: WHITMORE

First Name: MICHAEL

MI: J

Signature: _____

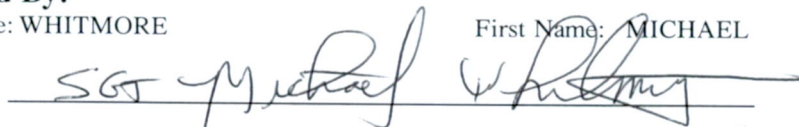

Badge No.: 215

Date: 11/04/2018

#215