

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWF-0359
Location:	LAWRENCE TWP POLICE	
Calibration File No.:	01236	Calib. No.: 00028
Certification File No.:	01237	Cert. No.: 00024
Linearity File No.:	01238	Lin. No.: 00024
Solution File No.:	01259	Soln. No.: 00213
Sequential File No.:	01259	File Date: 03/14/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWJ S3-0356
Solution Control Lot:	17200	Expires: 06/28/2019
		Bottle No.: 0515

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:23S		
Control 1 EC	0.102%	17:24S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	17:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:24S		
Control 2 EC	0.100%	17:25S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	17:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:26S		
Control 3 EC	0.100%	17:27S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	17:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:27S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: EVERIST

First Name: THOMAS

MI: J

Signature: \_\_\_\_\_

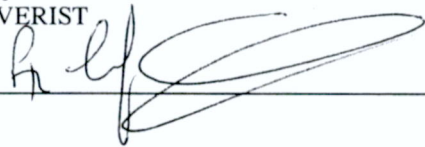

193

Badge No.: 193

Date: 03/14/2018