

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWF-0359
Location:	LAWRENCE TWP POLICE		
Calibration File No.:	01362	Calib. Date:	12/09/2019
Certification File No.:	01363	Cert. Date:	12/09/2019
Linearity File No.:	01364	Lin. Date:	12/09/2019
Solution File No.:	01374	Soln. Date:	04/02/2020
Sequential File No.:	01374	File Date:	04/02/2020
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWJ S3-0356
Solution Control Lot:	19240	Expires:	09/09/2021
		Bottle No.:	1367

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:39S		
Control 1 EC	0.099%	08:39S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:40S		
Control 2 EC	0.098%	08:41S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:42S		
Control 3 EC	0.098%	08:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:43S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: WHITMORE

First Name: MICHAEL

MI: J

Signature:

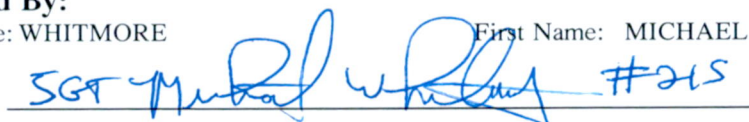

Badge No.: 215

Date: 04/02/2020