

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Location: LAWRENCE TWP POLICE
Serial No.: ARWF-0359
Calibration File No.: 01342
Calib. Date: 07/10/2019
Calib. No.: 00032
Certification File No.: 01313
Cert. Date: 01/30/2019
Cert. No.: 00027
Linearity File No.: 01314
Lin. Date: 01/30/2019
Lin. No.: 00027
Solution File No.: 01341
Soln. Date: 07/03/2019
Soln. No.: 00233
Sequential File No.: 01342
File Date: 07/10/2019


Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 18220
Model No.: CU-34
Serial No.: DDWJ S3-0355
Expires: 07/23/2020
Bottle No.: 0895

Coordinator

Last Name: GAMBONE
First Name: BRIAN
MI: M
Badge No.: 7029
Date: 07/10/2019
Signature: TPR T B M # 7029

*Black Key Temperature Probe Serial.....# DDMBP1-0016 (BMC)

*Digital NIST Temperature Measuring System Serial.....# 191959034 (BMC)

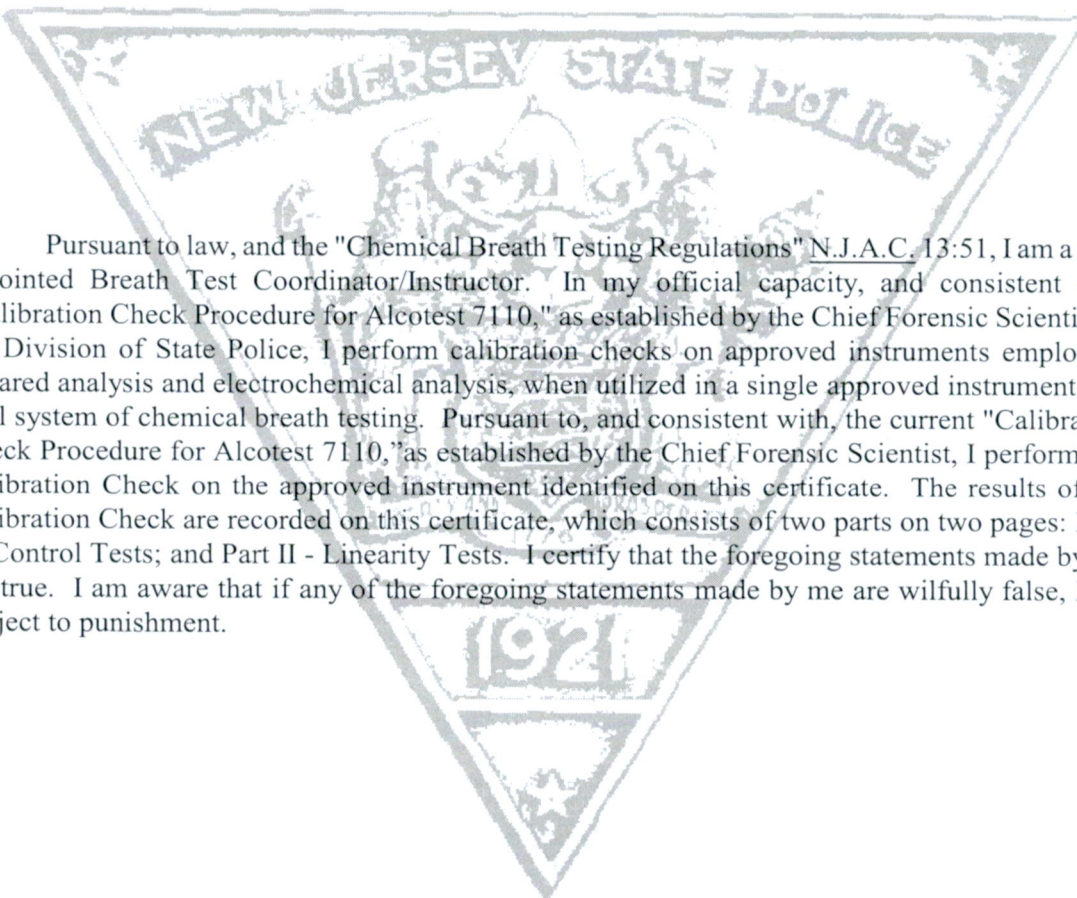

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWF-0359
Location: LAWRENCE TWP POLICE
Calibration File No.: 01342 Calib. Date: 07/10/2019 Calib. No.: 00032
Certification File No.: 01343 Cert. Date: 07/10/2019 Cert. No.: 00028
Linearity File No.: 01314 Lin. Date: 01/30/2019 Lin. No.: 00027
Solution File No.: 01341 Soln. Date: 07/03/2019 Soln. No.: 00233
Sequential File No.: 01343 File Date: 07/10/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWJ S3-0355
Control Solution %: 0.100% Expires: 07/23/2020
Solution Control Lot: 18220 Bottle No.: 0895

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:14D		
Control 1 EC	0.099%	09:14D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:15D		
Control 2 EC	0.099%	09:16D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:16D		
Control 3 EC	0.100%	09:17D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:18D		

All tests within acceptable tolerance.

Coordinator

Last Name: GAMBONE First Name: BRIAN MI: M
Signature: *Brian Gambone* #7029 Badge No.: 7029
Date: 07/10/2019

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWF-0359
Location: LAWRENCE TWP POLICE
Calibration File No.: 01342 Calib. Date: 07/10/2019 Calib. No.: 00032
Certification File No.: 01343 Cert. Date: 07/10/2019 Cert. No.: 00028
Linearity File No.: 01344 Lin. Date: 07/10/2019 Lin. No.: 00028
Solution File No.: 01341 Soln. Date: 07/03/2019 Soln. No.: 00233
Sequential File No.: 01344 File Date: 07/10/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDCB-0001
Control Solution %: 0.040% Expires: 07/31/2020
Solution Control Lot: 18240 Bottle No.: 1085

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAE-0016
Control Solution %: 0.080% Expires: 08/06/2020
Solution Control Lot: 18250 Bottle No.: 1122

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0005
Control Solution %: 0.160% Expires: 08/21/2020
Solution Control Lot: 18260 Bottle No.: 0694

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:28D		
Control 1 EC	0.041%	09:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	09:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:30D		
Control 2 EC	0.040%	09:31D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	09:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:32D		
Control 3 EC	0.082%	09:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	09:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:34D		
Control 4 EC	0.081%	09:35D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.080%	09:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:36D		
Control 5 EC	0.162%	09:37D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.160%	09:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:38D		
Control 6 EC	0.161%	09:39D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.160%	09:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:41D		

All tests within acceptable tolerance.

Coordinator

Last Name: GAMBONE

First Name: BRIAN

MI: M

Signature: Tpr. I Brian M [Signature] # 7029

Badge No.: 7029

Date: 07/10/2019

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWF-0359
Location: LAWRENCE TWP POLICE
Calibration File No.: 01342 Calib. Date: 07/10/2019 Calib. No.: 00032
Certification File No.: 01343 Cert. Date: 07/10/2019 Cert. No.: 00028
Linearity File No.: 01344 Lin. Date: 07/10/2019 Lin. No.: 00028
Solution File No.: 01345 Soln. Date: 07/10/2019 Soln. No.: 00234
Sequential File No.: 01345 File Date: 07/10/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWJ S3-0355
Control Solution %: 0.100% Expires: 01/31/2020
Solution Control Lot: 18050 Bottle No.: 0782

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:45D		
Control 1 EC	0.101%	10:46D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:46D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:47D		
Control 2 EC	0.100%	10:47D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:48D		
Control 3 EC	0.100%	10:49D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:49D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:49D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWAP2-213 

Changed By:

Last Name: GAMBONE First Name: BRIAN MI: M
Signature: TPA I Brian Gambone #7029 Badge No.: 7029
Date: 07/10/2019

**Alcotest 7110 MKIII-C Calibration
NIST-Traceable Digital Thermometer Readings**

Coordinator:

TPA-I Brian M. Gambone
Name

7029
Badge No.

Location:

Lawrence Twp Police
Agency

ARWF-0359
Alcotest Serial No.

Equipment:

191959034
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDCB-0001	08:04 D	09:05 D	34.0°C
0.08%	DDAE-0016	08:04 D	09:06 D	33.9°C
0.10%	DDWJ 53-0355	08:04 D	09:07 D	34.0°C
0.16%	DDAK 53-0005	08:04 D	09:08 D	34.0°C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius \pm 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

TPA-I B M Gambone # 7029
Coordinator's Signature

7/10/2019
Date

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

DDCB-0001

Certification Date:

5-30-19

Technician:

BS

Re-Certification Due Date:

5-30-20

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

DDAE-0016

Certification Date:

6-11-19

Technician:

BS

Re-Certification Due Date:

6-11-20

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDRK53-0005

Certification Date:

6-12-19

Technician:

BS

Re-Certification Due Date:

6-12-20

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDMBP1-0016

Certification Date:

6-10-19

Next Certification Due:

6-10-20

Probe Value:

102

Dräger, Inc.

BS



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-10177853

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601, S/N: 191959034 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath	93139		
Thermistor Module	A17118	20 Apr 2019	1000424560
Thermistor Module	A27129	10 Jan 2020	1000436202
Temperature Calibration Bath	A73332		
Temperature Probe	3039	08 May 2019	6-B7F4L-20-1
Temperature Calibration Bath	A79341		
Temperature Probe	5394	29 Jan 2020	B9124038
Temperature Calibration Bath	B16388		
Temperature Probe	5267	28 Jan 2020	B9124036

Certificate Information:

Technician: 104 Procedure: CAL-06 Cal Date: 13 Feb 2019 Cal Due Date: 13 Feb 2021
 Test Conditions: 38.85%RH 24.21°C 1023mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		-0.002	0.000	Y	-0.052	0.048	0.0087	>4:1
°C	N.A.	N.A.		24.999	25.000	Y	24.949	25.049	0.0087	>4:1
°C	N.A.	N.A.		50.001	50.001	Y	49.951	50.051	0.0087	>4:1
°C	N.A.	N.A.		100.002	100.002	Y	99.952	100.052	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement": (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max= As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Aaron Judice
Aaron Judice, Technical Manager

Note:

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
 Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.control3.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
 Control Company is ISO 9001:2008 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-RvA.
 International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-10177853

Traceable® Certificate of Calibration for Digital Thermometer

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.control3.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-RvA.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 07/31/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18220

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1210 to 0.1233 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 23, 2020.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Ali M. Alaouie, Ph.D.
Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 1st day of August, 2018.
Handwritten signature of Mary Elizabeth McLaughlin
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 08/28/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18240

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0486 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 31, 2020.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ali M. Alaoui]

Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 29th day of August, 2018.
[Mary Elizabeth McLaughlin signature]
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"
New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 08/30/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0976 to 0.0987 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 06, 2020.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Michael Kennedy

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 4th day of September, 2018.

Handwritten signature of Mary Elizabeth McLaughlin
Notary

MARY ELIZABETH MCLAUGHLIN

ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 09/13/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1938 to 0.1964 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 21, 2020.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18th day of September, 2018.

Mary E. McLaughlin
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



An Internationally Accredited Agency

New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 02/14/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18050

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1219 to 0.1229 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 31, 2020.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ali M. Alaouie]

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15th day of February, 2018.

[Handwritten signature of Mary E. McLaughlin]
Notary

MARY ELIZABETH MCLAUGHLIN

ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Traffic and Public Safety
Which is to certify that

Brian M. Gambone
Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL TESTS AND OTHER PROCEDURES PURSUANT TO A MASTER LICENSE
THE LAWS OF 1966 IN THE OPERATION OF THE ALCOHOL 7110 MKII-C
A METHOD TO DETERMINE BLOOD ALCOHOL
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 9th DAY OF October

TWO THOUSAND AND NINETY
[Signature] COLONEL NEW JERSEY STATE POLICE
[Signature] AT TRENTON, NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
11/19/18	GCFA	Adam Stankin
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2838 (Rev. 01/19)

DEPARTMENT OF
Traffic and Public Safety
Which is to certify that

Brian M. Gambone
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL TESTS AND OTHER PROCEDURES PURSUANT TO CHAPTER 12 OF
THE LAWS OF 1966 IN THE OPERATION OF THE ALCOHOL 7110 MKII-C
A METHOD TO DETERMINE BLOOD ALCOHOL
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 15th DAY OF July

TWO THOUSAND AND TEN
[Signature] SUPERVISOR NEW JERSEY STATE POLICE
[Signature] ATTORNEY GENERAL STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1/28/17	CCPA	Wm. Linn
11/4/14	CCPA	Adam Stankin
6/14/16	CCPA	Adam Stankin
11/19/18	GCFA	Adam Stankin
5.		
6.		
7.		
8.		
9.		

S.P. 2838 (Rev. 03/19)

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

3-16-15

SERIAL NUMBER:

ARWF-0359

Dräger Safety Diagnostics, Inc.

PC

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDW 353-0355

Certification Date:

4-19-19

Technician:

BS

Re-Certification Due Date:

4-19-20

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDWAP 2-213

Certification Date:

4-18-19

Next Certification Due:

4-18-20

Probe Value:

103

Draeger, Inc.

BS