

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWF-0359
Location:	LAWRENCE TWP POLICE	
Calibration File No.:	01263	Calib. Date: 04/09/2018
Certification File No.:	01264	Calib. No.: 00029
Linearity File No.:	01265	Cert. Date: 04/09/2018
Solution File No.:	01275	Cert. No.: 00025
Sequential File No.:	01275	Lin. Date: 04/09/2018
		Lin. No.: 00025
		Soln. Date: 08/06/2018
		Soln. No.: 00218
		File Date: 08/06/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWJ S3-0356
Solution Control Lot:	17200	Expires: 06/28/2019
		Bottle No.: 0645

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:07D		
Control 1 EC	0.100%	17:08D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	17:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:09D		
Control 2 EC	0.099%	17:09D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	17:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:10D		
Control 3 EC	0.098%	17:10D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	17:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: EVERIST

First Name: THOMAS

MI: J

Signature: \_\_\_\_\_

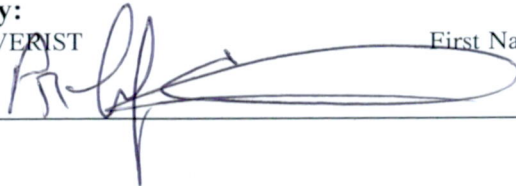

Badge No.: 193

Date: 08/06/2018