

Alcotest 7110 Calibration Record

Equipment


Alcotest 7110 MKIII-C
Location: LAWRENCE TWP POLICE
Serial No.: ARWF-0359
Calibration File No.: 01161
Calib. Date: 12/06/2016
Calib. No.: 00026
Certification File No.: 01108
Cert. Date: 06/09/2016
Cert. No.: 00021
Linearity File No.: 01109
Lin. Date: 06/09/2016
Lin. No.: 00021
Solution File No.: 01155
Soln. Date: 11/13/2016
Soln. No.: 00194
Sequential File No.: 01161
File Date: 12/06/2016

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 16220
Model No.: CU-34
Serial No.: DDWJ S3-0355
Expires: 09/07/2018
Bottle No.: 0491

Coordinator

Last Name: GONCALVES
First Name: MICHELLE
MI: L
Signature: Sgt. Michelle Goncalves #6040
Badge No.: 6040
Date: 12/06/2016

*Black Key Temperature Probe Serial.....# DDUNP2-237 (MA)
*Digital NIST Temperature Measuring System Serial.....# 150649677 (MA)

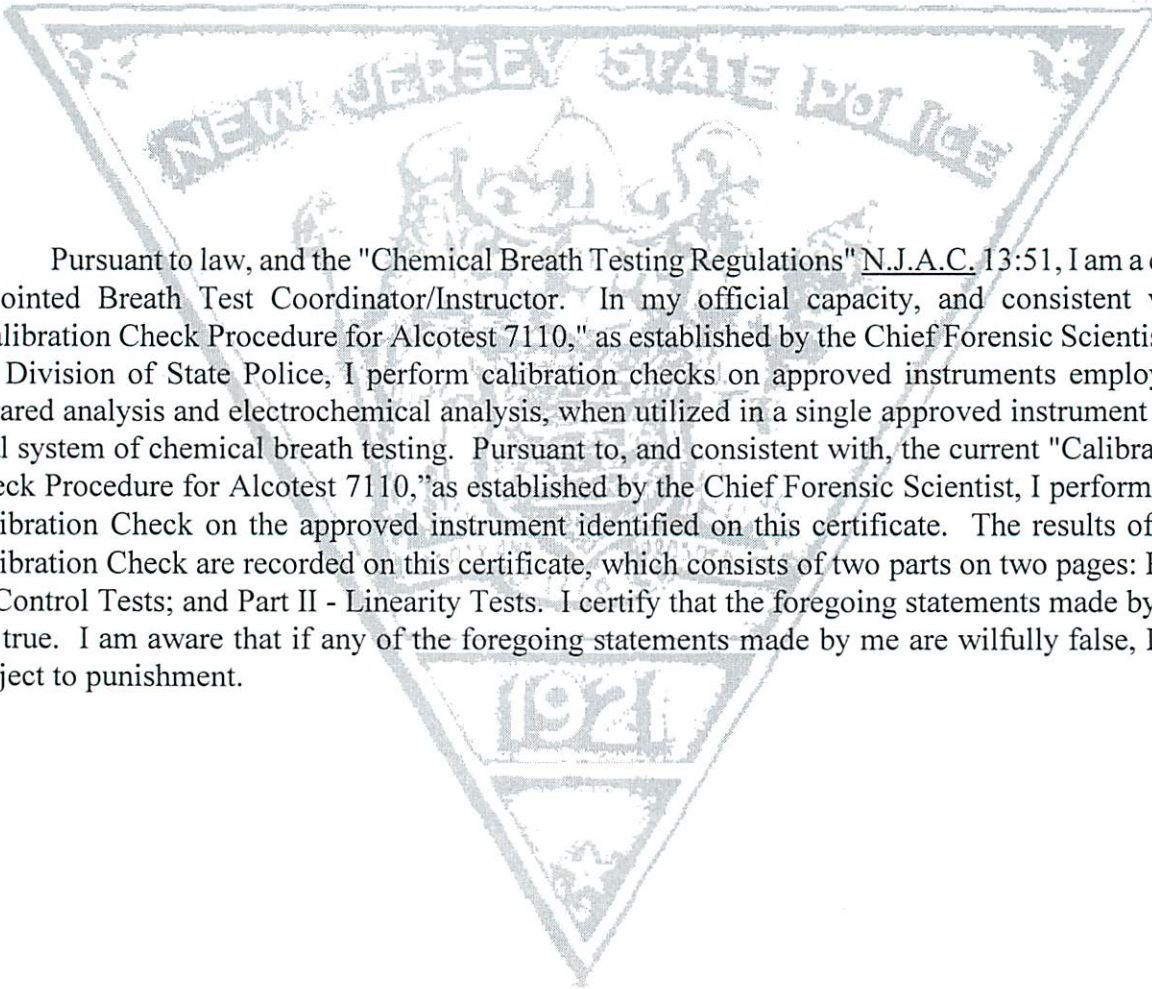

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWF-0359
Location: LAWRENCE TWP POLICE
Calibration File No.: 01161 Calib. Date: 12/06/2016 Calib. No.: 00026
Certification File No.: 01162 Cert. Date: 12/06/2016 Cert. No.: 00022
Linearity File No.: 01109 Lin. Date: 06/09/2016 Lin. No.: 00021
Solution File No.: 01155 Soln. Date: 11/13/2016 Soln. No.: 00194
Sequential File No.: 01162 File Date: 12/06/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWJ S3-0355
Control Solution %: 0.100% Expires: 09/07/2018
Solution Control Lot: 16220 Bottle No.: 0491

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:46S		
Control 1 EC	0.100%	10:46S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:47S		
Control 2 EC	0.099%	10:48S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:49S		
Control 3 EC	0.099%	10:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:50S		

All tests within acceptable tolerance.

Coordinator

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: Sgt Michelle Goncalves #6040

Badge No.: 6040

Date: 12/06/2016

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWF-0359
Location: LAWRENCE TWP POLICE
Calibration File No.: 01161 Calib. Date: 12/06/2016 Calib. No.: 00026
Certification File No.: 01162 Cert. Date: 12/06/2016 Cert. No.: 00022
Linearity File No.: 01163 Lin. Date: 12/06/2016 Lin. No.: 00022
Solution File No.: 01155 Soln. Date: 11/13/2016 Soln. No.: 00194
Sequential File No.: 01163 File Date: 12/06/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDMK S3-0003
Control Solution %: 0.040% Expires: 09/19/2018
Solution Control Lot: 16230 Bottle No.: 1403

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0193
Control Solution %: 0.080% Expires: 09/27/2018
Solution Control Lot: 16250 Bottle No.: 0671

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDCN-0052
Control Solution %: 0.160% Expires: 10/03/2018
Solution Control Lot: 16260 Bottle No.: 1015

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:23S		
Control 1 EC	0.042%	11:23S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.042%	11:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:25S		
Control 2 EC	0.041%	11:25S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	11:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:27S		
Control 3 EC	0.082%	11:27S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.081%	11:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:29S		
Control 4 EC	0.081%	11:30S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.080%	11:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:31S		
Control 5 EC	0.163%	11:32S	34.0°C	*** TEST PASSED ***
Control 5 IR	0.161%	11:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:33S		
Control 6 EC	0.161%	11:34S	34.0°C	*** TEST PASSED ***
Control 6 IR	0.160%	11:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:36S		

All tests within acceptable tolerance.

Coordinator

Last Name: GONCALVES


First Name: MICHELLE

MI: L

Signature: Sgt. Michelle Delo # 6040

Badge No.: 6040

Date: 12/06/2016



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDWJS3-0355

Certification Date

Technician

Re-Certification Due Date

11-01-16

LAG

11-01-17

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDWAPL-213

11-03-16

11-03-17

Probe Value

103

Draeger Safety Diagnostics, Inc.
Technical Service Department

LAG

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:
3-16-15

SERIAL NUMBER:
ARWF-0359

Dräger Safety Diagnostics, Inc.

PC



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor
KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General
COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 08/08/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16150

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1200 to 0.1210 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 06, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Signature of Ali M. Alaouiie, Ph.D.
Ali M. Alaouiie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 9th day of August, 2016.

Signature of Mary Elizabeth McLaughlin
Notary
MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





Calibration
Certificate No. 1750.01

Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-7019767

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087

Instrument Identification:

Model: 61220-601 S/N: 150649677 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-256	B01375		
Temperature Probe	128	4/02/16	15-A0P2S-40-1
Thermistor Module	A17118	3/03/16	1000371058
Temperature Calibration Bath TC-179	A45240		
Thermistor Module	A17118	3/03/16	1000371058
Temperature Probe	3039	4/02/16	15-A0P2S-20-1
Temperature Calibration Bath TC-231	A79341		
Thermistor Module	A27129	11/04/15	1000365407
Temperature Probe	5202	11/19/16	6-CV9Y2-1-1
Temperature Calibration Bath TC-309	B3A444		
Thermistor Module	A27129	11/04/15	1000365407
Temperature Probe	5267	11/19/16	6-CV9Y0-1-1

Certificate Information:

Technician: 68 Procedure: CAL-06 Cal Date: 8/31/15 Due Date: 8/31/17
 Test Conditions: 23.0°C 47.0 %RH 1017 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		0.001	0.000	Y	-0.049	0.051	0.013	3.8:1
°C		N.A.		25.000	25.001	Y	24.950	25.050	0.014	3.6:1
°C		N.A.		50.004	50.000	Y	49.954	50.054	0.014	3.6:1
°C		N.A.		100.002	99.999	Y	99.952	100.052	0.014	3.6:1

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy= $\pm(\text{Max}-\text{Min})/2$; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Aaron Judice
Aaron Judice, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA
 Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
 Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2008-AQ-HOU-RvA.
 International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

DEPARTMENT OF
Traffic and Public Safety
What is to certify that

Michelle L. Gonçalves
 New Jersey State Police

IS QUALIFIED AND COMPEtent TO CONDUCT COURSE IN ACCORDANCE WITH PURSUANT TO CHAPTER 142 OF
 THE LAWS OF IN THE OPERATION OF THE Alcotest 7110 MKIII-C
 A METHOD TO DEFENSE IN EDUCATION
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, 15th DAY OF December

TWO THOUSAND AND Eleven

[Signature]
 SUPERINTENDENT
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 12-3-13	GCPA	Wm horns
2. 9/17/15	GCPA	Adrian S. Dore
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 03/10)

DEPARTMENT OF
Traffic and Public Safety
What is to certify that

Michelle Gonçalves
 New Jersey State Police

IS QUALIFIED AND COMPEtent TO CONDUCT COURSE IN ACCORDANCE WITH PURSUANT TO CHAPTER 142 OF
 THE LAWS OF IN THE OPERATION OF THE Breath Test Coordinator/Instructor
 A METHOD TO DEFENSE IN EDUCATION
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, 23rd DAY OF March

TWO THOUSAND AND Twelve


[Signature]
 SUPERINTENDENT
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 02/12)



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDMKS3-0003

Certification Date

9-28-16

Technician

72

Re-Certification Due Date

9-28-17



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDCN-0052

Certification Date


9-28-16

Technician

72

Re-Certification Due Date

9-28-17



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDXDS3-0193

Certification Date

Technician

Re-Certification Due Date

09-27-16

RAJ

9-27-17

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDUNP2-237

9-30-16

9-30-17

Probe Value

105

Draeger Safety Diagnostics, Inc.
Technical Service Department

BC



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 582-2000

CHRISTOPHER S. POKRINO
Attorney General

COLONEL JOSEPH R. FURNIES
Superintendent

CHRIS CHRISTIE
Governor

KIM GUADAÑO
Lt. Governor

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 09/19/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16220

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1202 to 0.1207 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 07, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Signature]
Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 19th day of September, 2016.

[Signature]
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"
New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08623-0068
(609) 882-2000

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.


ANALYSIS DATE: 09/27/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16230


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0484 to 0.0492 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 19, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

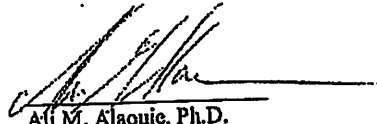
Ali M. Alaoui, Ph.D,
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28th day of September, 2016.


Notary
MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

CHRISTOPHER S. PORRINO
Attorney General

KIM GUADAGNO
Lt. Governor

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/04/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0965 to 0.0975 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 27, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Signature]
Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 5th day of October, 2016.

[Signature]
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/13/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1928 to 0.1964 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 3, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 17 day of October, 2016.

Notary
JOHN R LEAVER
ID # 2207138
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 14, 2017



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer.
Printed on Recycled Paper and Recyclable



Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWF-0359
Location:	LAWRENCE TWP POLICE	
Calibration File No.:	01161	Calib. Date: 12/06/2016
Certification File No.:	01162	Calib. No.: 00026
Linearity File No.:	01163	Cert. Date: 12/06/2016
Solution File No.:	01169	Cert. No.: 00022
Sequential File No.:	01169	Lin. Date: 12/06/2016
		Lin. No.: 00022
		Soln. Date: 12/30/2016
		Soln. No.: 00196
		File Date: 12/30/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWJ S3-0355
Solution Control Lot:	201609A	Expires: 09/07/2018
		Bottle No.: 1485

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:24S		
Control 1 EC	0.101%	01:25S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	01:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:26S		
Control 2 EC	0.100%	01:26S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	01:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:27S		
Control 3 EC	0.100%	01:28S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	01:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:29S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WHITMORE

First Name: MICHAEL

MI: J

Signature: SG Michael Whitmore

Badge No.: 215

Date: 12/30/2016

#215

DEPARTMENT OF
Traffic and Public Safety
 This is to certify that

Michael J. Whitmore
Lawrence Township

QUALIFIED AND EMPLOYED AS AN OPERATOR OF BREATH ANALYSIS EQUIPMENT IN CHAPTER 142 OF
 TITLE 17C, N.J.A.C. IN THE OPERATING TIME Alcotest 7110 MKIII-C
 ON THE DATE OF EXAMINATION IN THE YEAR 2014 AT Fort
 MONROE, NEW JERSEY THIS 13th DAY OF April
 BETWEEN THE YEARS AND thirteen

 COMMISSIONER
 NEW JERSEY STATE POLICE

 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

	DATE	Refresher Course PLACE	INSTRUCTOR
1.	2/2/15	ULPA	Adam [Signature]
2.			
3.			
4.			
5.			
6.			
7.			
8.			
9.			
10.			

S.P. 233B (Rev. 02/12)

ORIGINAL COURSE DATES 12/01/2004

DATE	Refresher Course PLACE	INSTRUCTOR
1. 1/15/2009	Morris Co. P.A.	Snyder
2. 1/6/11	OLPA	Adam Standa
3. 1/2/13	OLPA	Adam Standa
4. 1/21/15	OLPA	Adam Standa
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 07/07)

DEPARTMENT OF
Law and Public Safety
This is to certify that

Steven Simon

Lawrence Township Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 143 OF

THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 7110 MK III-C

A METHOD TO DETERMINE INTOXICATION. GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 26th DAY OF February

TWO THOUSAND AND Nine


SUPERINTENDENT
NEW JERSEY STATE POLICE


ATTORNEY GENERAL
STATE OF NEW JERSEY

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWF-0359
Location: LAWRENCE TWP POLICE
Calibration File No.: 01161 **Calib. Date:** 12/06/2016 **Calib. No.:** 00026
Certification File No.: 01162 **Cert. Date:** 12/06/2016 **Cert. No.:** 00022
Linearity File No.: 01163 **Lin. Date:** 12/06/2016 **Lin. No.:** 00022
Solution File No.: 01179 **Soln. Date:** 02/21/2017 **Soln. No.:** 00198
Sequential File No.: 01179 **File Date:** 02/21/2017

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWJ S3-0355
Control Solution %: 0.100% **Expires:** 09/07/2018
Solution Control Lot: 201609A **Bottle No.:** 1483

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:42S		
Control 1 EC	0.102%	18:43S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	18:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:44S		
Control 2 EC	0.100%	18:44S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	18:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:45S		
Control 3 EC	0.102%	18:46S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	18:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:47S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WHITMORE

First Name: MICHAEL

MI: J

Signature:  #215

Badge No.: 215

Date: 02/21/2017

DEPARTMENT OF
Law and Public Safety
 This is to certify that

Michael J. Whitmore
Lawrence Township

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
 THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 7110 MKIII-C
 A METHOD TO DETERMINE INTOXICATION.
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 4th DAY OF April

TWO THOUSAND AND Thirteen

[Signature]
 SUPERINTENDENT
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____

	DATE	Refreshers Course PLACE	INSTRUCTOR
1.	<u>2/2/15</u>	<u>OLCPA</u>	<u>Adam Stamba</u>
2.	<u>1/18/17</u>	<u>LAKEHURST</u>	<u>Adam Stamba</u>
3.	_____	_____	_____
4.	_____	_____	_____
5.	_____	_____	_____
6.	_____	_____	_____
7.	_____	_____	_____
8.	_____	_____	_____
9.	_____	_____	_____